

A11103 070664

MENT OF

NAT'L INST OF STANDARDS & TECH R.I.C.



A1103070664

United States. Natio/Interagency compar
QC100 .U57 NO.529 1978 C.2 NBS-PUB-C 197



BUREAU OF STANDARDS

NBS SPECIAL PUBLICATION

529

U.S. DEPARTMENT OF COMMERCE / National Bureau of Standards

Interagency Comparison of Ultraviolet Photometric Standards for Measuring Ozone Concentrations

QC
100
U57
NO.529
1978
C.2

NATIONAL BUREAU OF STANDARDS

The National Bureau of Standards¹ was established by an act of Congress March 3, 1901. The Bureau's overall goal is to strengthen and advance the Nation's science and technology and facilitate their effective application for public benefit. To this end, the Bureau conducts research and provides: (1) a basis for the Nation's physical measurement system, (2) scientific and technological services for industry and government, (3) a technical basis for equity in trade, and (4) technical services to promote public safety. The Bureau's technical work is performed by the National Measurement Laboratory, the National Engineering Laboratory, and the Institute for Computer Sciences and Technology.

THE NATIONAL MEASUREMENT LABORATORY provides the national system of physical and chemical and materials measurement; coordinates the system with measurement systems of other nations and furnishes essential services leading to accurate and uniform physical and chemical measurement throughout the Nation's scientific community, industry, and commerce; conducts materials research leading to improved methods of measurement, standards, and data on the properties of materials needed by industry, commerce, educational institutions, and Government; provides advisory and research services to other Government Agencies; develops, produces, and distributes Standard Reference Materials; and provides calibration services. The Laboratory consists of the following centers:

Absolute Physical Quantities² — Radiation Research — Thermodynamics and Molecular Science — Analytical Chemistry — Materials Science.

THE NATIONAL ENGINEERING LABORATORY provides technology and technical services to users in the public and private sectors to address national needs and to solve national problems in the public interest; conducts research in engineering and applied science in support of objectives in these efforts; builds and maintains competence in the necessary disciplines required to carry out this research and technical service; develops engineering data and measurement capabilities; provides engineering measurement traceability services; develops test methods and proposes engineering standards and code changes; develops and proposes new engineering practices; and develops and improves mechanisms to transfer results of its research to the ultimate user. The Laboratory consists of the following centers:

Applied Mathematics — Electronics and Electrical Engineering² — Mechanical Engineering and Process Technology² — Building Technology — Fire Research — Consumer Product Technology — Field Methods.

THE INSTITUTE FOR COMPUTER SCIENCES AND TECHNOLOGY conducts research and provides scientific and technical services to aid Federal Agencies in the selection, acquisition, application, and use of computer technology to improve effectiveness and economy in Government operations in accordance with Public Law 89-306 (40 U.S.C. 759), relevant Executive Orders, and other directives; carries out this mission by managing the Federal Information Processing Standards Program, developing Federal ADP standards guidelines, and managing Federal participation in ADP voluntary standardization activities; provides scientific and technological advisory services and assistance to Federal Agencies; and provides the technical foundation for computer-related policies of the Federal Government. The Institute consists of the following divisions:

Systems and Software — Computer Systems Engineering — Information Technology.

¹Headquarters and Laboratories at Gaithersburg, Maryland, unless otherwise noted; mailing address Washington, D.C. 20234.

²Some divisions within the center are located at Boulder, Colorado, 80303.

JAN 2 1979

Lab Acc. Cur.

60100

1039

10. 2-4

1978

c 2

Interagency Comparison of Ultraviolet Photometric Standards for Measuring Ozone Concentrations

Wendt,¹ J. Kowalski,¹ A. M. Bass,²
Ellis,³ and M. Patapoff⁴

California Air Resources Board
Emeryville, California 94608

National Measurement Laboratory
National Bureau of Standards
Washington, DC 20234

Environmental Protection Agency
Research Triangle Park
Durham, North Carolina 27709

Propulsion Laboratory
Pasadena, California 91104



U.S. DEPARTMENT OF COMMERCE, Juanita M. Kreps, Secretary

Jordan J. Baruch, Assistant Secretary for Science and Technology

NATIONAL BUREAU OF STANDARDS, Ernest Ambler, Director

Issued December 1978

Library of Congress Catalog Card Number: 78-600126

National Bureau of Standards Special Publication 529

Nat. Bur. Stand. (U.S.), Spec. Publ. 529, 25 pages (Dec. 1978)

CODEN: XNBSAV

U.S. GOVERNMENT PRINTING OFFICE

WASHINGTON: 1978

For sale by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402

Stock No. 003-003-02002-8 Price \$1.30

(Add 25 percent additional for other than U.S. mailing).

Interagency Comparison of Ultraviolet Photometric Standards for Measuring Ozone Concentrations

J. Wendt, J. Kowalski, A. M. Bass, C. Ellis, and M. Patapoff

ABSTRACT

In August 1977, an interlaboratory comparison study was initiated after the California Air Resources Board and the Environmental Protection Agency, Research Triangle Park independently designed and constructed ozone absolute ultraviolet photometers. These units augmented the photometers already designed and in use by the National Bureau of Standards and the Jet Propulsion Laboratory. Previous ozone comparisons involving indometry, ultraviolet photometry and gas phase titration have reported results differing by as much as $\pm 30\%$. The protocol of this study, performed at the California Air Resources Board, Haagen-Smit Laboratory, El Monte, was a multipoint comparison using the NBS photometer as the standard. The results of the data analysis indicate excellent agreement with a total variation of 2.8%. Compared to the NBS photometer the EPA-RTP photometer read 1.3% low, the JPL photometer read 1.5% high and the ARB photometer read 0.4% low. The correlation coefficients of the same data sets were 1.0000, 1.0000 and 0.9999 respectively.

Key words: Air pollution; atmospheric monitoring; calibration; ozone; ultraviolet; photometry.

1. INTRODUCTION

For more than 100 years, ozone concentrations have been determined by utilizing the chemical reaction between ozone and potassium iodide to liberate iodine which is then measured by chemical or physical means. The neutral buffered, potassium iodide (NBKI) method has gained wide acceptance and is the calibration technique of the Federal Reference Method for measuring photochemical oxidant concentrations.[6] Despite variations in the chemical composition of the reagents, all of the potassium iodide methods in common use assume a one to one stoichiometry between the iodine released and the ozone reacted.[2]

Studies conducted by the California Air Resources Board and the U. S. Environmental Protection Agency have shown significant departures from the assumed stoichiometry. The stoichiometry departures were found to depend on the buffering agent and potassium iodide concentrations. These departures also depend on the nature of the buffering agent and the absolute humidity of the sample air stream.[2,3]

As a result of the various studies, the California Air Resources Board in May of 1975 adopted ultraviolet photometry as its reference method for measuring ozone concentrations.[7] Since California's adoption, interest in ultraviolet photometry as a standard for measuring ozone concentrations has steadily escalated. Ultraviolet photometry is now generally considered a prime candidate for replacing the existing

¹Figures in brackets indicate literature references at the end of this paper.

NBKI calibration procedure and ASTM Methods for measuring photochemical ozone concentrations.

By June of 1977, four agencies, the California Air Resources Board, National Bureau of Standards, U. S. Environmental Protection Agency, and the Jet Propulsion Laboratory independently designed and fabricated long path ultraviolet ozone photometers. The four photometers are all of different design with two located on each coast of the United States.

In August of 1977 the photometers or suitable transfer standards were assembled at the California Air Resources Board's Laboratory in El Monte, California. The four photometric standards were allowed to sample a common ozone supply and their respective readings compared. The results of the comparison are reported.

2. PHOTOMETER DESIGNS

2.1 National Bureau of Standards (NBS)

The NBS photometer is designed to measure ozone concentrations ranging from 0.05 to 10.0 ppm with an accuracy of approximately 0.005 ppm by volume. The design of the photometer, shown in figure 1, incorporates a double-beam arrangement to provide greater precision in the measurement by elimination of variability in the UV source. The cells of the photometer are approximately 3 meters long and are made of 1-1/2" diameter pyrex pipe; teflon gaskets are used to make vacuum-tight seals for the fused silica windows. The light from a low pressure mercury discharge lamp is passed through a narrow-band interference filter in order to isolate the 253.7 nm emission line. The light is collimated by a fused silica lens and passed through a partially-transmitting neutral density filter which serves as a beam splitter. The two beams then pass through

the two absorption cells. Adjustable aperture stops limit the diameter of the beams to ensure that there are no reflections from inner walls of the cells. The light beams emerge from the cells and are recombined on the face of a photomultiplier tube by another partially reflecting filter.

Light passing through each sample cell is alternately allowed to fall on the photomultiplier by means of a light chopper. A chopper blade with a single hole is driven by a hysteresis synchronous motor. Light emitting diode-phototransistor pairs are used to sense the positioning of the hole in the chopper blade; the signal from the phototransistor triggers a discriminator to start the timing and counting cycle for each sample tube.

A logic system, triggered by the discriminators, controls pulse counters associated with each sample tube. In order to ensure precise counting times as the photomultiplier is exposed to each tube, an electronic gate is used to ensure that the photomultiplier is fully (and not merely partly) exposed to the light beam passing through the sample.

The pulse output from the photomultiplier is amplified, and pulse counting is performed by conventional 100 MHz pulse counters and a rough guide of overall pulse rate is provided by a rate meter. Counting time is determined by a preset counter. At the end of a counting interval, the results are printed out.

House air, dried and filtered, flows through one cell ("reference cell"), then into an ozone generator from which ozonized air flows through the second cell ("sample cell"). The measurement is made by comparing the ratio of the signals transmitted by the two cells in the

presence and in the absence of ozone. This provides the transmittance ($Tr = \frac{I}{I_0}$), and the ozone concentration is determined by application of the Beer-Lambert Law. Since the mercury lamp is viewed, nearly simultaneously, through both cells, fluctuations in lamp intensity do not affect the measurement. Any impurity present in the air stream will be observed in both cells and will not interfere with the O_3 determination,[8] unless it too is photolysed by the O_3 generator and it or the products absorb at 253.7 nm.

2.2 Jet Propulsion Laboratory (JPL)

There are three components to the JPL photometer, the light source, the absorption cell, and the light detector as shown in figure 2. A low-pressure mercury lamp is used as a source of the 253.7 nm light. A 1/4-m monochromator was used to spectrally isolate the 253.7 nm line. (This component is not strictly necessary and can be replaced by an interference filter to isolate the 253.7 nm line). Collimation of the light beam was aided by use of a 25-cm focal length quartz lens. Stability of the light source was enhanced by operation from a constant voltage transformer and by enclosing the lamp in an aluminum block for increased thermal inertia. The absorption cell is constructed of 2-in o.d. Pyrex tubing, and has a path length of 5.00 m. Quartz windows are attached at each end by means of epoxy cement, with care being taken to minimize internal exposure of cement. The 253.7 nm light emerging from the cell is monitored with a solar-blind, side-on photomultiplier tube. The photomultiplier is operated at 340 V. The photomultiplier output voltage is measured across a 10-M Ω resistor and is read with a four-

digit voltmeter. A 0.4- μ fd condensor is placed in parallel with the resistor to obtain a suitable time constant.

Ozone is generated in a stream of cylinder air by means of a photochemical generator of conventional design, employing a low-pressure mercury lamp with a sliding shield to vary the O_3 concentration. The gas flow through the cell, usually 5-7 l/min, enters near one end of the cell and exits at the opposite end. It has been established experimentally that there is no appreciable gradient of ozone concentration in the cell.

With carrier gas flowing, photomultiplier output voltages are read periodically during the calibration procedure and are plotted as a function of time. At intervals, transmittance readings are taken at ozone concentrations in the range 0.00 to 0.85 ppm of O_3 . Transmittance ratios (I_0/I_t) are then calculated, and ozone concentrations determined by application of the Beer-Lambert Law.[9]

2.3 Environmental Protection Agency (EPA-RTP)

The EPA-RTP photometer, as shown in figure 3, is a two meter instrument designed to demonstrate how off-the-shelf electronics could be used to produce a high precision (± 1 ppb) photometer. The absorption volume consists of two one-meter cells in a folded path configuration which reduces the overall instrument length to 1.27 meters and greatly improves the system's portability. The cells are made of 12 mm inside diameter pyrex tubing and are fitted with quartz windows via teflon gaskets. The optical path is folded by means of small plane mirrors which are located outside the absorption cell.

The photometer is essentially monochromatic due to use of a Vycor envelope on the low pressure mercury source and solar blind vacuum photo-diode detectors. A reference detector is used to monitor the light source in a quasi-double beam configuration. A sample detector is used to monitor the absorption of the light in the cell.

An ozone concentration is determined by alternately filling the cell with ozone-free reference air and the ozone calibration atmosphere. The transmittance of the ozone sample is equal to the ratio of the normalized sample channel frequency obtained with ozone in the absorption cell to that obtained with reference air in the cell. The ozone concentration is calculated from the transmittance via the Beer-Lambert absorption law.

2.4 California Air Resources Board (ARB)

The ARB photometer is designed to measure ozone concentrations ranging from 0.02 to 15.0 ppm with an accuracy of 0.01 ppm over the entire range. To achieve the design accuracy, the photometer incorporates a double beam principle which eliminates errors resulting from light source or air supply variations. The cells of the photometer are constructed from 1/2 inch diameter Pyrex pipe with a path length of 260 centimeters. Quartz windows, sealed with epoxy cement, are affixed to each end of the cells as shown in figure 4.

A low pressure mercury discharge lamp of sufficient length to span both cells of the photometer is used as a source of 253.7 nm light. The Vycor sheath of the lamp and the detector spectral response characteristics limit the photometer sensitivity to the 253.7 nm emission line. Lamp output stability is achieved by operating the mercury discharge lamp

from a crystal controlled, chopped d.c. power supply, and housing the lamp in a thermally controlled aluminum block.

Light passing through the sample and reference cells is converted to analog current signals by separate detectors mounted in a thermally controlled aluminum block. The analog current signals are converted to frequency signals utilizing digital electrometers. The electrometer outputs are connected to a dual channel frequency counter capable of counting the reference channel to a preset value. Each time the preset reference count is reached, the ratio of the sample detector count to reference detector count is displayed.

An ozone concentration measurement is accomplished by first admitting ozone free air to each cell of the photometer. The ratio $I_0/\text{REFERENCE INTENSITY}$ (ratio of zero air to reference detector count) is recorded. Ozonized air from the ozone generator is then admitted to the sample cell with ozone free air flowing through the reference cell. The ratio $I/\text{REFERENCE INTENSITY}$ (ratio of sample to reference detector count) is recorded and the transmittance ratio I/I_0 calculated. The ozone concentration is calculated from the Beer-Lambert Law.

3. EXPERIMENTAL

The experimental phase of the photometer comparison was conducted at the California Air Resources Board's El Monte Laboratory utilizing the experimental setup of figure 5. Clean, dry, ozone free air was supplied to the experimental setup by an Aadco clean air supply designed to ARB specifications. The clean air was metered to a Monitor Labs Inc. Model 8500 calibration system and to a multiported glass manifold by mass flow controllers. The ozone output of the calibration system was

ducted to a multiported glass manifold. All interconnections were made using Teflon tubing.

A direct comparison of the NBS and JPL photometers with those of the ARB and EPA-RTP could not be accomplished due to the large size, complexity and construction characteristics of the photometers. NBS and JPL participation in the comparison studies was accomplished through the use of Dasibi Corporation Model 1003 AH ozone monitors[10] as transfer standards. Each transfer standard was calibrated against the respective agencies' photometer before and after the El Monte comparison. Both the ARB and EPA-RTP photometer, described herein, were used directly in the comparison studies. It should be noted that the EPA-RTP photometer was disassembled, shipped, and reassembled at the ARB laboratories. With minimal checkout prior to the comparison, the precision and stability the readings were less than in previous laboratory measurements.

A total of eight experimental runs, each consisting of pre and post run instrument zero, and an ozone concentration ranging from 0.05 to 0.70 ppm, were completed. Following each experimental run, the respective agencies calculated the ozone concentration recorded by their photometer by making the necessary temperature and pressure adjustments using the following equations:

ARB, EPA-RTP*

$$C \text{ (ppm)} = \frac{(10^6)}{(K)} \frac{(760)}{(L)} \frac{(T)}{(P)} \frac{(273)}{(273)} \ln \frac{I_o}{I}$$

where:

T = absolute temperature, °K

P = absolute pressure in photometer, torr

L = photometer path length, cm

k = extinction coefficient, base e, $\text{cm}^{-1} \text{atm}^{-1}$

I_0 = intensity of light with zero ozone

I = intensity of light with ozone at concentration

* The EPA-RTP calculations also include a 1% correction for ozone losses which occur in the photometer.[11]

JPL

$$C \text{ (ppm)} = \frac{(127.098) (\beta) (T)}{(P)} \ln \frac{100 - \frac{B}{0.539}}{100 - \frac{R}{0.539}} \quad [12]$$

where:

β = correction constant for reference Dasibi S/N 1386; (1.0685)

B = Dasibi background reading

R = Dasibi ozone reading

P = absolute pressure, torr

T = absolute temperature, °K

NBS

$$C \text{ (ppm)} = \frac{(127.098) (\beta) (T)}{(P)} \ln \frac{54.6}{54.6 - \Delta I} \quad [13]$$

where:

ΔI = change in light intensity between zero and ozonized air;
Dasibi reading)

T = absolute temperature, °K

P = absolute pressure, torr

β = correction constant for reference Dasibi S/N 1707; (1.0134)

54.6 = span factor of Dasibi transfer standard

The extinction coefficient used by all participants in the comparison study was $308.5 \text{ cm}^{-1} \text{ atm}^{-1}$ base e.[14]

4. RESULTS

The final ozone concentrations for each participant are tabulated as follows:

TABLE I
Ozone Concentrations
(Part per million)

Data Pt.	NBS	EPA-RTP	JPL	ARB
1	0.689	0.683	0.700	0.681
2	0.109	0.110	0.112	0.109
3	0.605	0.597	0.612	0.599
4	0.185	0.184	0.189	0.183
5	0.494	0.490	0.503	0.494
6	0.301	0.299	0.307	0.296
7	0.389	0.385	0.396	0.389
8	0.047	0.049	0.047	0.042

The NBS photometer was selected as the reference standard in the data analysis. As indicated in Table I the data show excellent agreement. A linear regression and correlation coefficient (r) analysis of the data confirms the agreement. From the analysis, the following relationships were obtained:

$$[O_3]_{NBS} = (1.013) [O_3]_{EPA-RTP} - (0.002) \quad r = 1.0000$$

$$[O_3]_{NBS} = (0.985) [O_3]_{JPL} - (0.001) \quad r = 1.0000$$

$$[O_3]_{NBS} = (1.004) [O_3]_{ARB} - (0.002) \quad r = 0.9999$$

Figures 6, 7, and 8 are linear regression plots of the NBS ozone concentrations versus the EPA-RTP, JPL, and ARB ozone concentrations.

It should be emphasized that for the comparison, both NBS and JPL utilized transfer standards, rather than the actual absolute photometers. Additionally the EPA-RTP photometer was shipped from North Carolina and assembled at the ARB laboratory with a minimum of checkout. The ARB photometer was the only unit compared in its stationary position. With this realization, the agreement to within 2.8% of all four units is highly significant.

The analysis indicates an excellent agreement utilizing the ultra-violet photometric techniques. The linear regression confirmed the accuracy of each method, with the correlation coefficients indicating a high degree of precision.

5. ACKNOWLEDGMENT

The authors wish to thank Drs. Jimmie Hodgeson (NBS), Richard Paur (EPA-RTP) and William DeMore (JPL) for their technical assistance and support of these studies. In addition, the authors thank Jolene Hori, Kevin Kalthoff, Jack Horrocks, and Kahirup Torre of the California Air Resources Board for their assistance throughout various phases of this effort.

This work was supported in part by the National Bureau of Standards' Office of Environmental Measurements Program.

6. REFERENCES

1. Hodgeson, J. A., "A Survey of Calibration Techniques for Atmospheric Ozone Monitors," NBSIR 76-1191, National Bureau of Standards, Washington, DC, December 1976.
2. DeMore, W. B., Romanovski, J. C., Feldstein, M., Hamming, W. J., Mueller, P. K., "Comparison of Oxidant Calibration Procedures", Ad Hoc Oxidant Measurement Committee, California Air Resources Board, February 3, 1975.
3. Torre, K. J., "A Study of the Effect of Atmospheric Humidity on Analytical Oxidant Measurement Methods", presented at 15th Conference - Methods in Air Pollution Studies, AIHL, Calif. Dept. of Health, Air Resources Board, Long Beach, Calif., Jan. 14-15, 1976.
4. DeMore, W. B., Patapoff, M., "Comparison of Ozone Determinations by Ultraviolet Photometry and Gas-Phase Titration", Environmental Science and Technology, 10, 897 (1976).
5. Flamm, D. L., "Analysis of Ozone at Low Concentrations with Boric Acid Buffered KI", Environmental Science and Technology 11, 978 (1977).
6. Federal Register, 36 (228), 22392 (Nov. 25, 1971).
7. State of California Air Resources Board Resolution 75-30, Board meeting, May 15, 1975, Sacramento, Calif.
8. Bass, A. M., Ledford, A. E. Jr., and Whittaker, J. K., NBS paper, "Ultraviolet Photometer for Ozone Calibration, in Methods and Standards for Environmental Measurement" (NBS Special Publication 464) 9-15 (1977).
9. DeMore, W. B., "Ozone Determination by Ultraviolet Absorption Photometry", presented at 15th Conference - Methods in Air Pollution Studies, AIHL, Calif. Dept. of Health, Air Resources Board, Long Beach, Calif., Jan. 14-15, 1976.
10. Bowman, L. D., Horak, R. F., "A Continuous Ultraviolet Absorption Ozone Photometer", ISA AID, 72430 (103-108) 1972.
11. Ellis, C., Southern California Edison Company, Rosemead, California, private communication, Oct. 1977.
12. Patapoff, M., Jet Propulsion Laboratory, Pasadena, California, private communication, Sept. 1977.
13. Bass, A. M., United States Department of Commerce, NBS, Washington, DC, private communication, Feb. 1978.

14. The value of k used in this work ($308.5 \text{ cm}^{-1} \text{ atm}^{-1}$) is based on an evaluation by R. Hampson and D. Garvin of measurements reported in the published literature:
- (a) Inn, E. C. Y. and Y. Tanaka, J. Opt. Soc. Am. 43, 870 (1953).
 - (b) Hearn, A. G., Proc. Phys. Soc. 78, 932 (1961).
 - (c) DeMore, W. B. and O. Raper, J. Phys. Chem. 68, 412 (1964).
 - (d) Griggs, M., J. Chem. Phys. 49, 857 (1968).
 - (e) Simons, J. W., R. J. Paur, H. A. Webster and E. J. Bair, J. Chem. Phys. 59, 1203 (1973).
 - (f) Becker, K. H., U. Schurath, and H. Seitz, Int. J. Chem. Kinet. 6, 725 (1974).

Disclaimer:

Certain trade names and company products are identified in order to adequately specify the experimental procedure. In no case does such identification imply recommendation or endorsement by the National Bureau of Standards, nor does it imply that the products are necessarily the best available for the purpose.

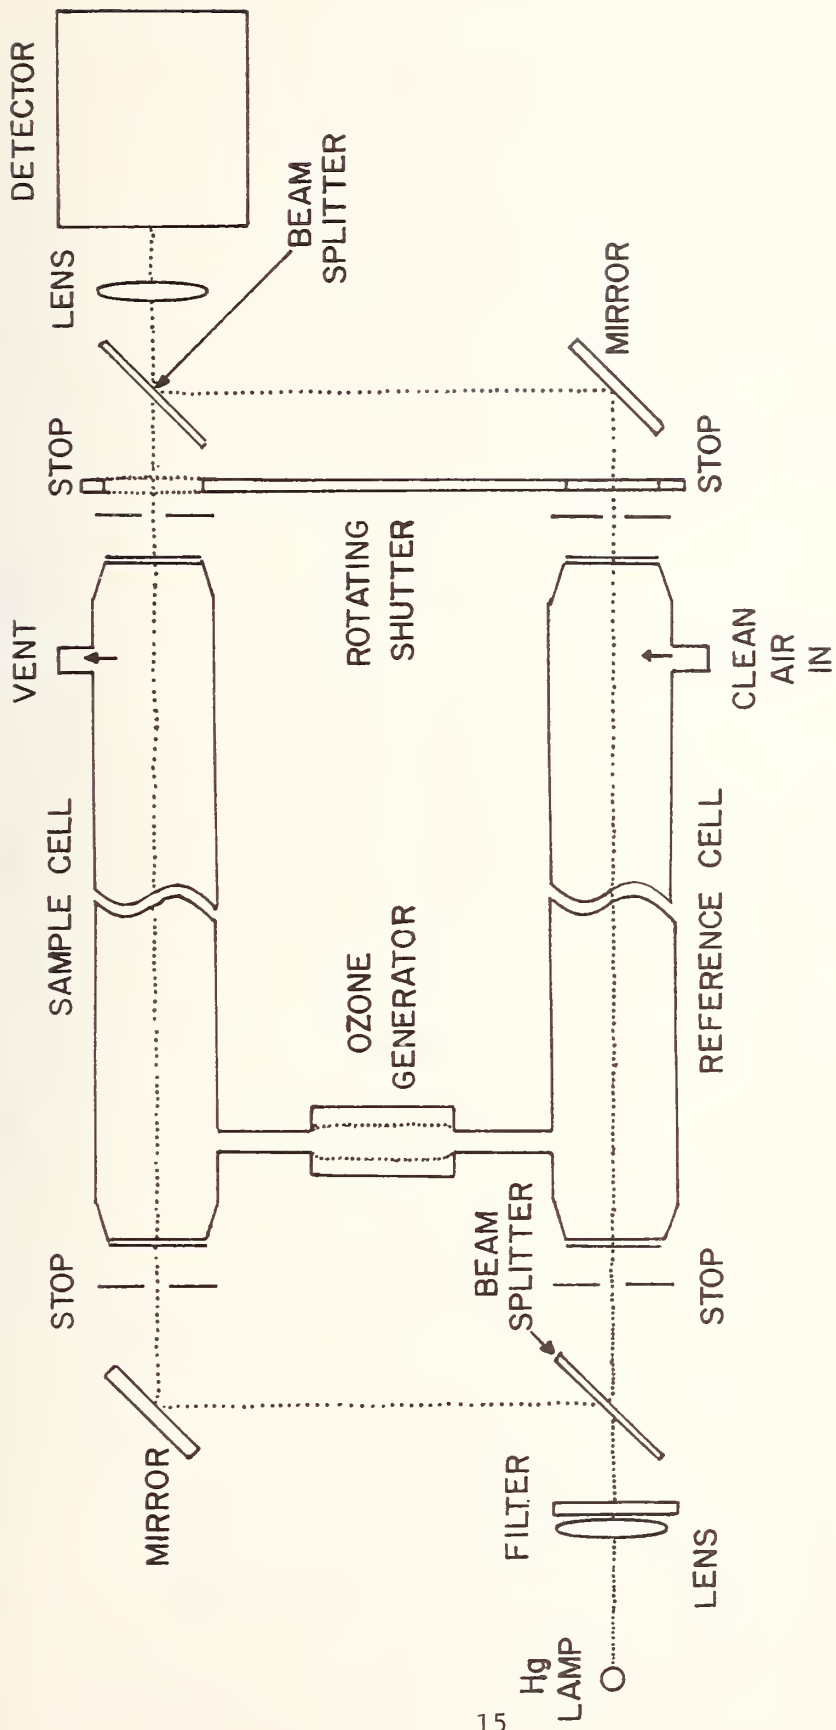


FIGURE 1 NBS ABSOLUTE PHOTOMETER

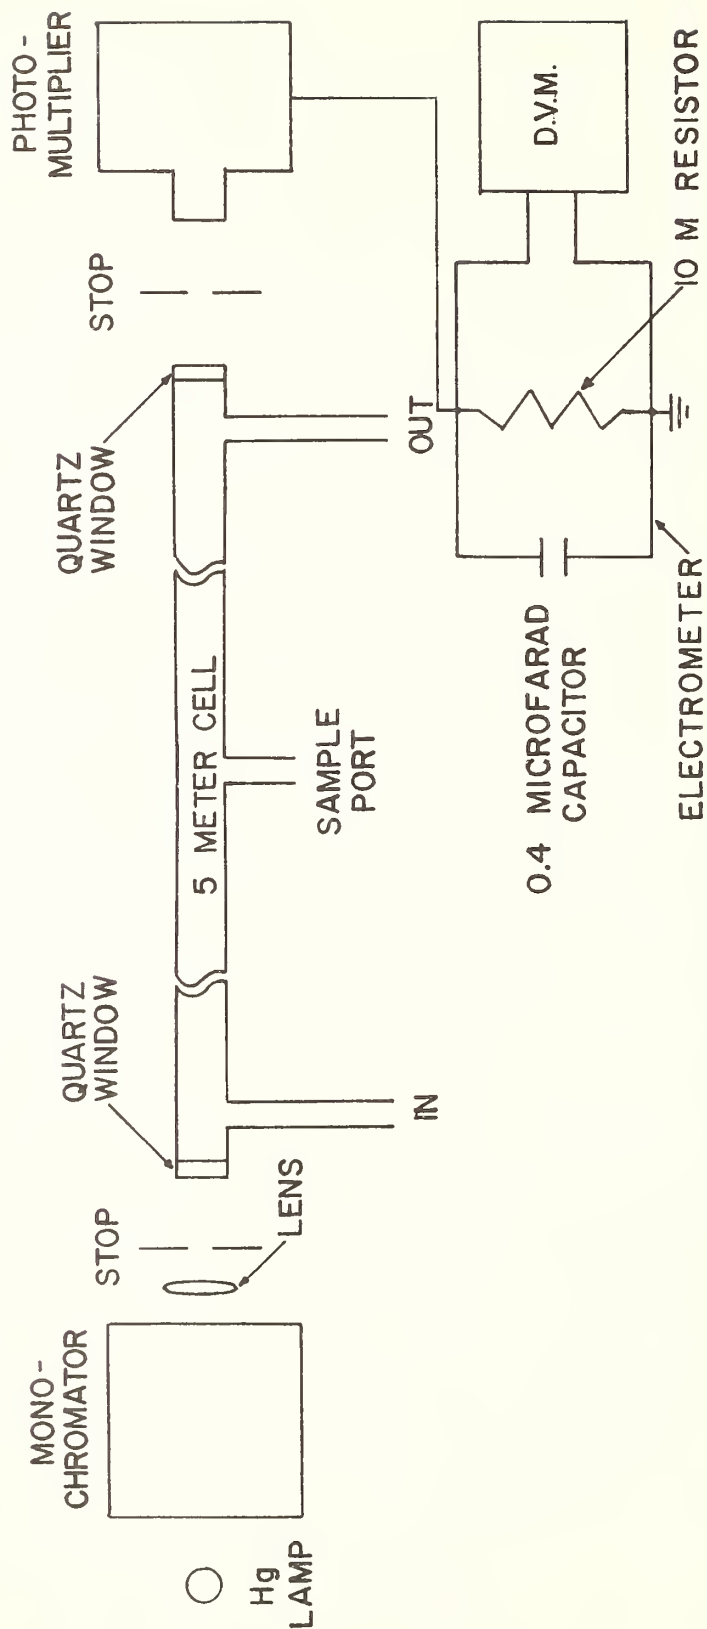


FIGURE 2 JPL ABSOLUTE PHOTOMETER

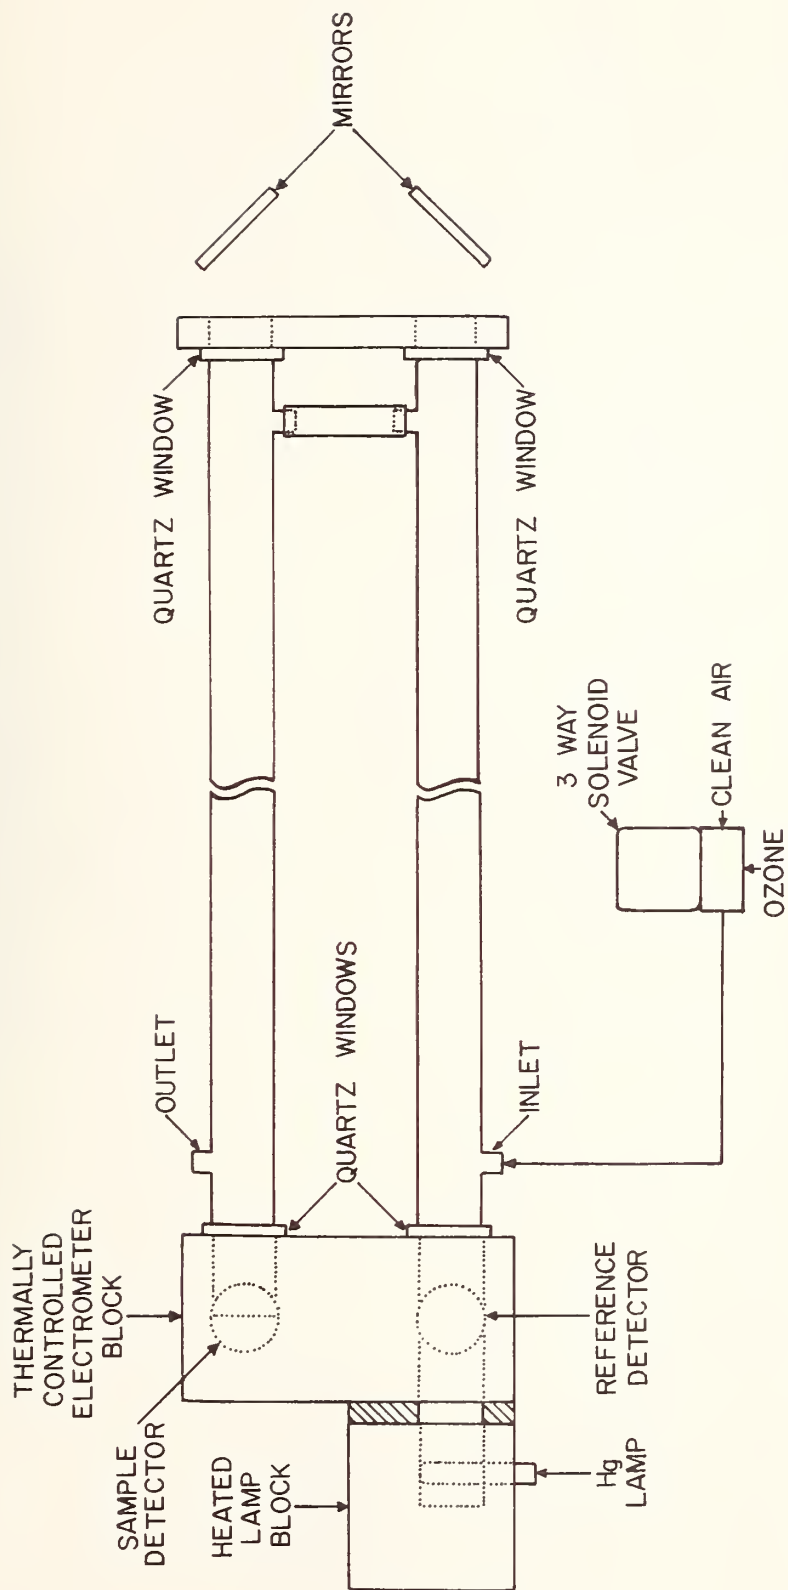


FIGURE 3 EPA ABSOLUTE PHOTOMETER

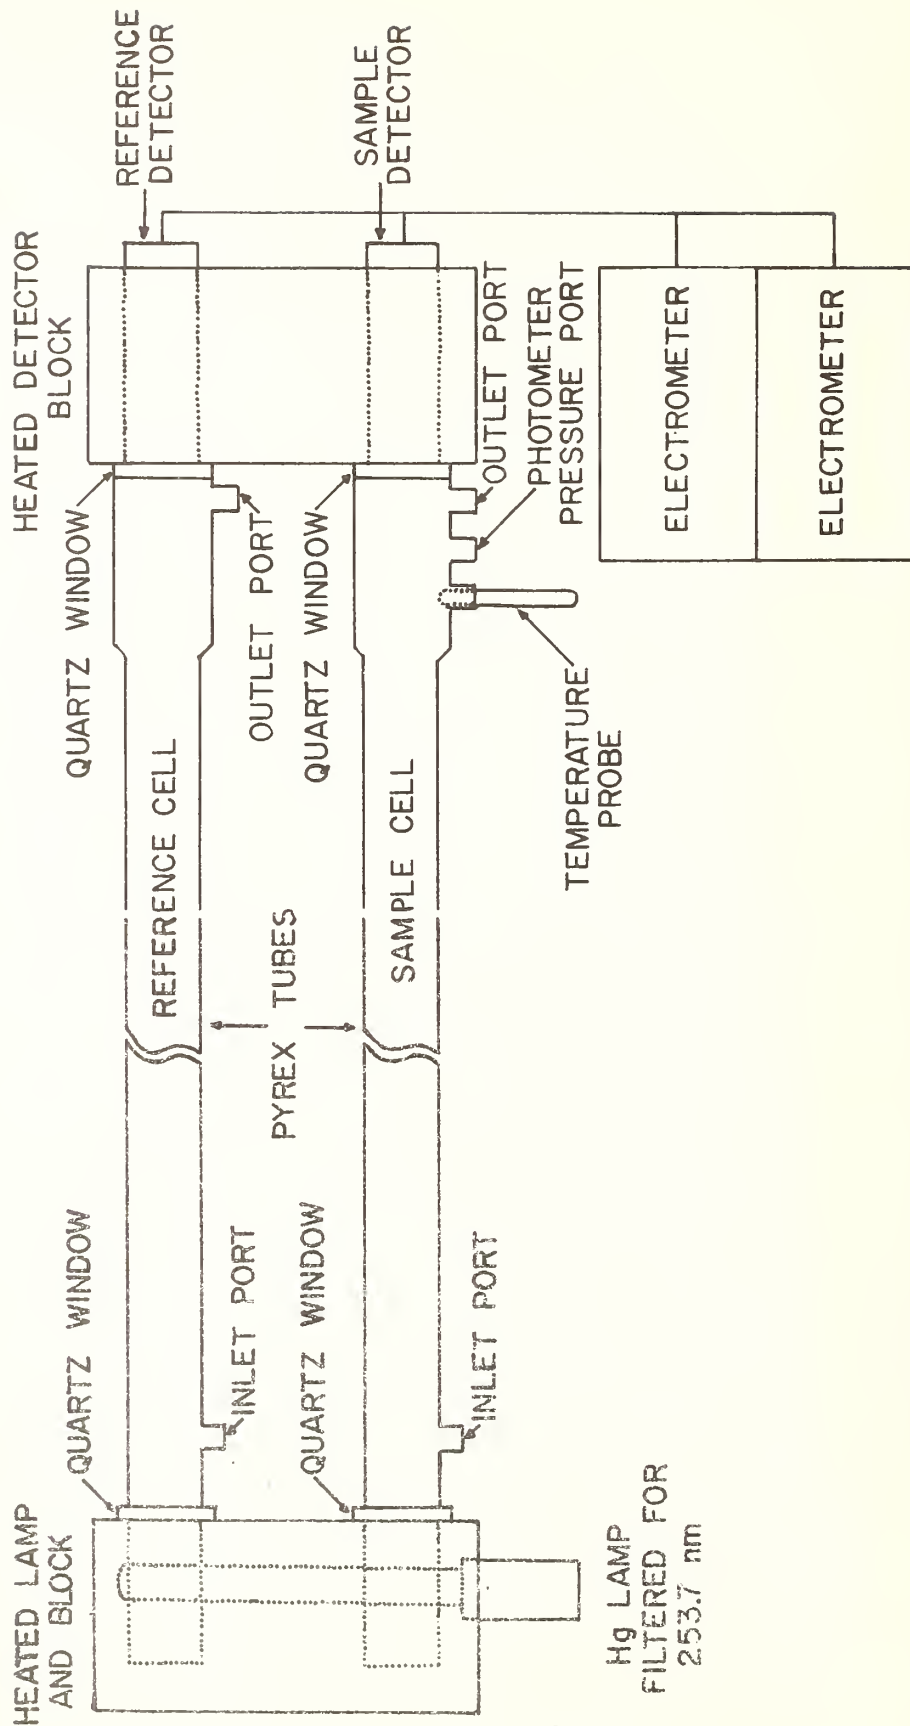


FIGURE 4 ARB ABSOLUTE PHOTOMETER

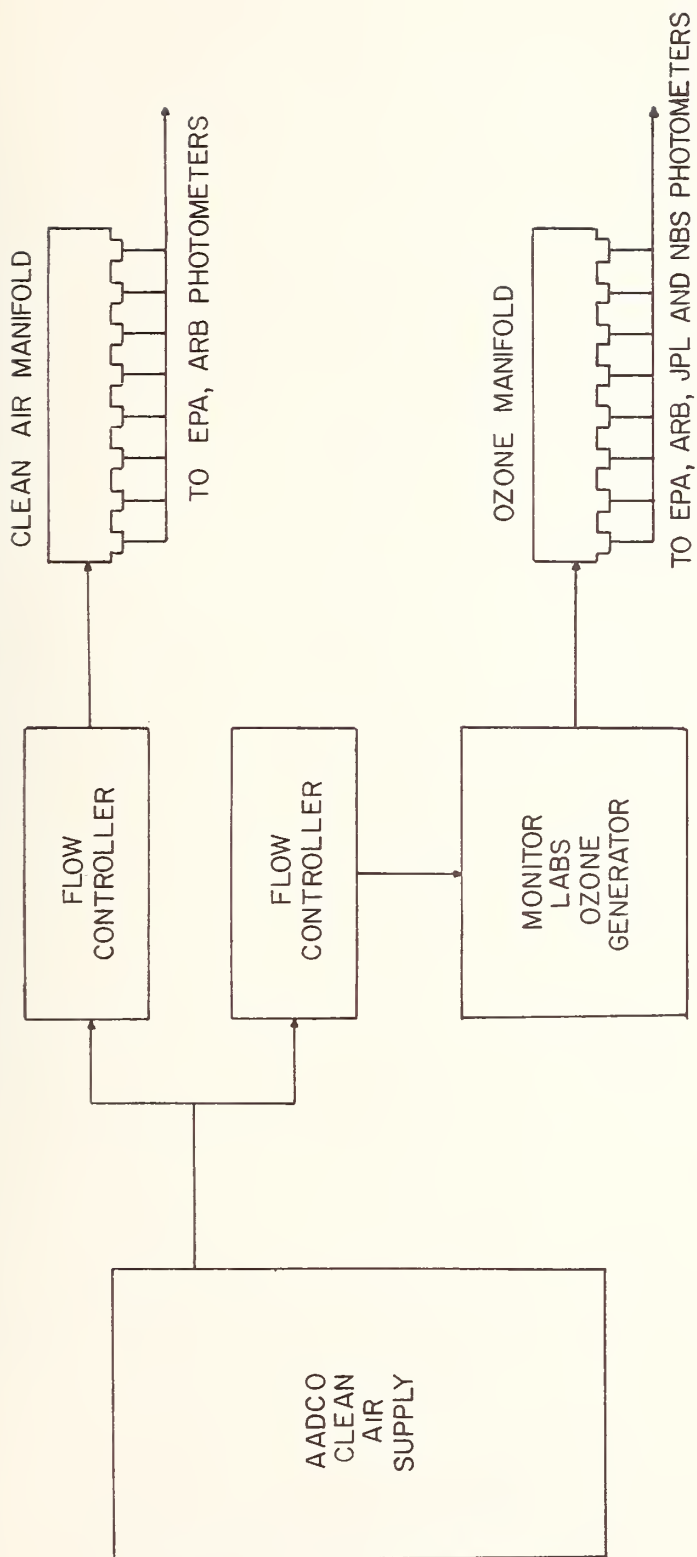


FIGURE 5 ZERO AIR AND OZONE SOURCES

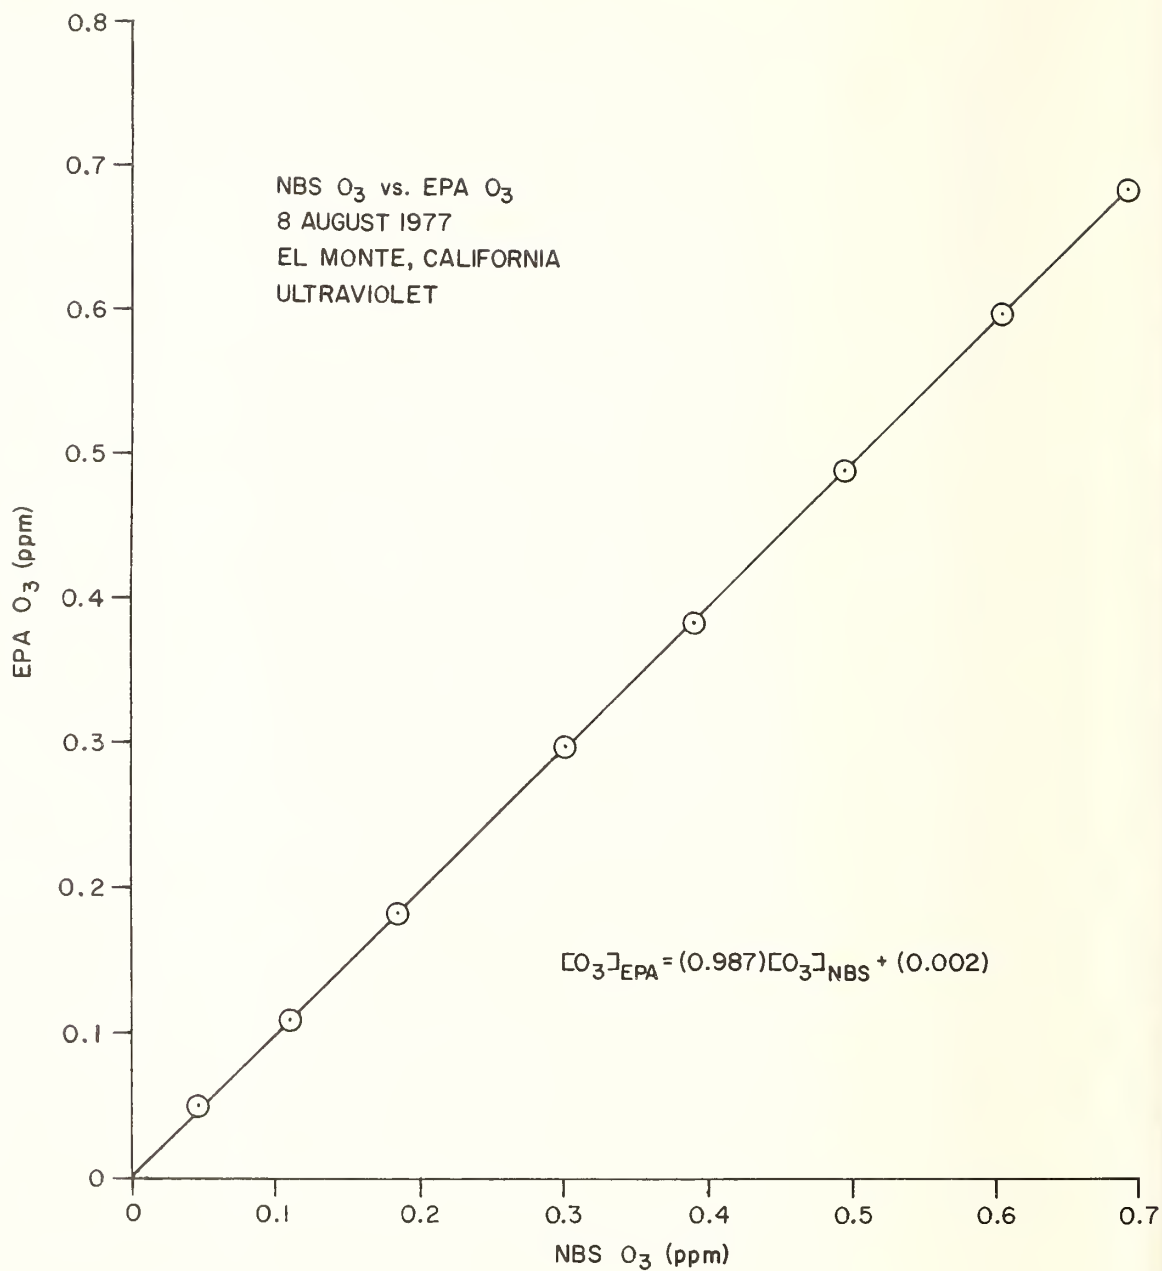


FIGURE 6

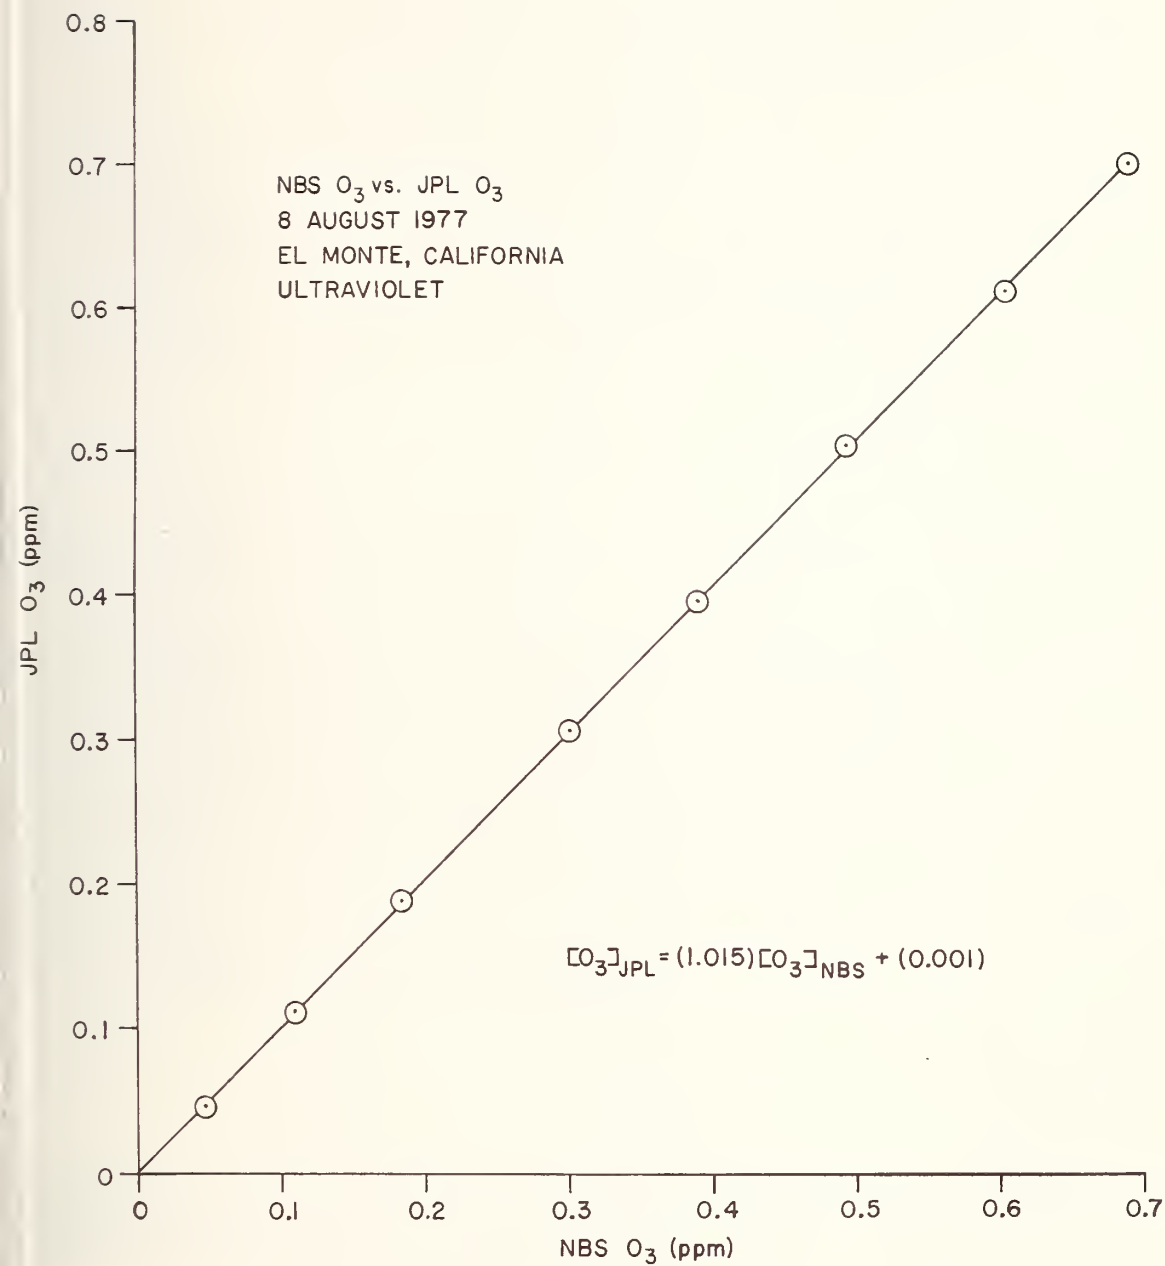


FIGURE 7


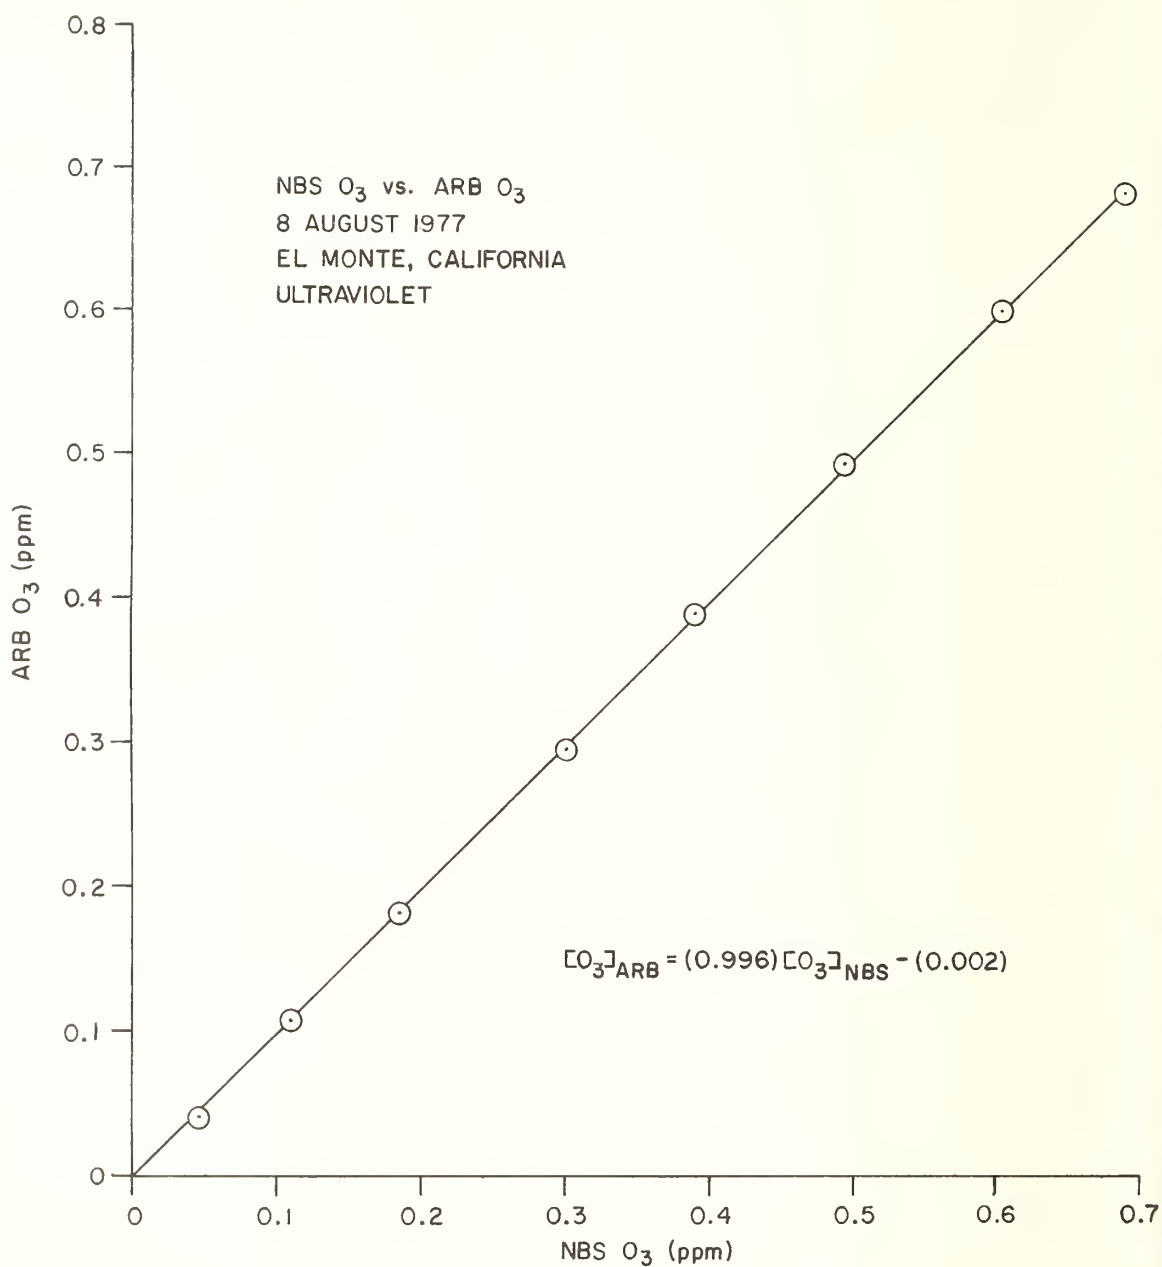


FIGURE 8

U.S. DEPT. OF COMM. BIBLIOGRAPHIC DATA SHEET	1. PUBLICATION OR REPORT NO. NBS SP 529	2. Gov't Accession No.	3. Recipient's Accession No.
4. TITLE AND SUBTITLE Interagency Comparison of Ultraviolet Photometric Standards for Measuring Ozone Concentrations		5. Publication Date December 1978	
		6. Performing Organization Code	
7. AUTHOR(S) J. Wendt, J. Kowalski, A. M. Bass, C. Ellis, M. Patapoff		8. Performing Organ. Report No.	
9. PERFORMING ORGANIZATION NAME AND ADDRESS NATIONAL BUREAU OF STANDARDS DEPARTMENT OF COMMERCE WASHINGTON, D.C. 20234		10. Project/Task/Work Unit No.	
		11. Contract/Grant No.	
12. Sponsoring Organization Name and Complete Address (Street, City, State, ZIP)		13. Type of Report & Period Covered	
		14. Sponsoring Agency Code	
15. SUPPLEMENTARY NOTES Library of Congress Catalog Card Number: 78-600126			
16. ABSTRACT (A 200-word or less factual summary of most significant information. If document includes a significant bibliography or literature survey, mention it here.) In August 1977, an interlaboratory comparison study was initiated after the California Air Resources Board and the Environmental Protection Agency, Research Triangle Park independently designed and constructed ozone absolute ultraviolet photometers. These units augmented the photometers already designed and in use by the National Bureau of Standards and the Jet Propulsion Laboratory. Previous ozone comparisons involving indometry, ultraviolet photometry and gas phase titration have reported results differing by as much as $\pm 30\%$. The protocol of this study, performed at the California Air Resources Board, Haagen-Smit Laboratory, El Monte, was a multi-point comparison using the NBS photometer as the standard. The results of the data analysis indicate excellent agreement with a total variation of 2.8%. Compared to the NBS photometer the EPA-RTP photometer read 1.3% low, the JPL photometer read 1.5% high and the ARB photometer read 0.4% low. The correlation coefficients of the same data sets were 1.0000, 1.0000 and 0.9999 respectively.			
17. KEY WORDS (six to twelve entries; alphabetical order; capitalize only the first letter of the first key word unless a proper name; separated by semicolons) Air pollution; atmospheric monitoring; calibration; ozone; ultraviolet photometry			
18. AVAILABILITY <input type="checkbox"/> Unlimited <input type="checkbox"/> For Official Distribution. Do Not Release to NTIS <input type="checkbox"/> Order From Sup. of Doc., U.S. Government Printing Office Washington, D.C. 20402, SD Cat. No. <u>003-003-</u> <input type="checkbox"/> Order From National Technical Information Service (NTIS) Springfield, Virginia 22151		19. SECURITY CLASS (THIS REPORT) UNCLASSIFIED	21. NO. OF PAGES 25
		20. SECURITY CLASS (THIS PAGE) UNCLASSIFIED	22. Price \$1.30

JOURNAL OF RESEARCH

of the National Bureau of Standards

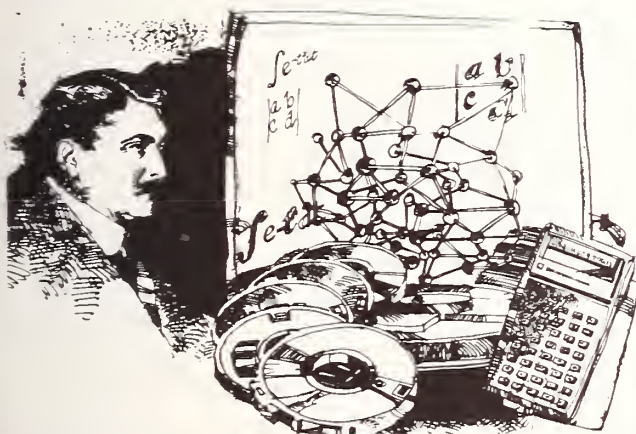

Subscribe now — The new National Bureau of Standards Journal

The expanded Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology, and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent NBS publications in NBS and non-NBS media. Issued six times a year. Annual subscription: domestic \$17.00; foreign \$21.25. Single copy, \$3.00 domestic; \$3.75 foreign.

- Note: The Journal was formerly published in two sections: Section A "Physics and Chemistry" and Section B "Mathematical Sciences."

NBS Board of Editors
Churchill Eisenhart,
Executive Editor (Mathematics)
John W. Cooper (Physics)
Donald D. Wagman (Chemistry)
Andrew J. Fowell (Engineering)
Joseph O. Harrison (Computer Science)
Stephen J. Smith (Boulder Labs.)

For a review copy, write Journal of Research, National Bureau of Standards, U.S. DEPARTMENT OF COMMERCE Washington, D.C. 20234

Subscription Order Form

Enter my subscription to NBS Journal of Research at \$17.00. Add \$4.25 for foreign mailing. No additional postage is required for mailing within the United States or its possessions. (SJR—File Code 2Q)

Send Subscription to:

Name-First, Last		
Company Name or Additional Address Line		
Street Address		
City	State	Zip Code

☐ Remittance Enclosed
(Make checks payable to Superintendent of Documents)

☐ Charge to my Deposit Account No.

MAIL ORDER FORM TO:
Superintendent of Documents
Government Printing Office
Washington, D.C. 20402

NBS TECHNICAL PUBLICATIONS

PERIODICALS

JOURNAL OF RESEARCH—The Journal of Research of the National Bureau of Standards reports NBS research and development in those disciplines of the physical and engineering sciences in which the Bureau is active. These include physics, chemistry, engineering, mathematics, and computer sciences. Papers cover a broad range of subjects, with major emphasis on measurement methodology, and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Bureau's technical and scientific programs. As a special service to subscribers each issue contains complete citations to all recent NBS publications in NBS and non-NBS media. Issued six times a year. Annual subscription: Domestic \$17.00; foreign \$21.25. Single copy, \$3.00 domestic; \$3.75 foreign.

Note: The Journal was formerly published in two sections: Section A "Physics and Chemistry" and Section B "Mathematical Sciences."

DIMENSIONS/NBS

This monthly magazine is published to inform scientists, engineers, businessmen, industry, teachers, students, and consumers of the latest advances in science and technology, with primary emphasis on the work at NBS. The magazine highlights and reviews such issues as energy research, fire protection, building technology, metric conversion, pollution abatement, health and safety, and consumer product performance. In addition, it reports the results of Bureau programs in measurement standards and techniques, properties of matter and materials, engineering standards and services, instrumentation, and automatic data processing.

Annual subscription: Domestic, \$11.00; Foreign \$13.75

NONPERIODICALS

Monographs—Major contributions to the technical literature on various subjects related to the Bureau's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NBS, NBS annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

Applied Mathematics Series—Mathematical tables, manuals, and studies of special interest to physicists, engineers, chemists, biologists, mathematicians, computer programmers, and others engaged in scientific and technical work.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a world-wide program coordinated by NBS. Program under authority of National Standard Data Act (Public Law 90-396).

NOTE: At present the principal publication outlet for these data is the Journal of Physical and Chemical Reference Data (JPCRD) published quarterly for NBS by the American Chemical Society (ACS) and the American Institute of Physics (AIP). Subscriptions, reprints, and supplements available from ACS, 1155 Sixteenth St. N.W., Wash., D.C. 20056.

Building Science Series—Disseminates technical information developed at the Bureau on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NBS under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The purpose of the standards is to establish nationally recognized requirements for products, and to provide all concerned interests with a basis for common understanding of the characteristics of the products. NBS administers this program as a supplement to the activities of the private sector standardizing organizations.

Consumer Information Series—Practical information, based on NBS research and experience, covering areas of interest to the consumer. Easily understandable language and illustrations provide useful background knowledge for shopping in today's technological marketplace.

Order above NBS publications from: Superintendent of Documents, Government Printing Office, Washington, D.C. 20402.

Order following NBS publications—NBSIR's and FIPS from the National Technical Information Services, Springfield, Va. 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. Register serves as the official source of information in the Federal Government regarding standards issued by NBS pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NBS Interagency Reports (NBSIR)—A special series of interim or final reports on work performed by NBS for outside sponsors (both government and non-government). In general, initial distribution is handled by the sponsor; public distribution is by the National Technical Information Services (Springfield, Va. 22161) in paper copy or microfiche form.

BIBLIOGRAPHIC SUBSCRIPTION SERVICES

The following current-awareness and literature-survey bibliographies are issued periodically by the Bureau:

Cryogenic Data Center Current Awareness Service. A literature survey issued biweekly. Annual subscription: Domestic, \$25.00; Foreign, \$30.00.

Liquefied Natural Gas. A literature survey issued quarterly. Annual subscription: \$20.00.

Superconducting Devices and Materials. A literature survey issued quarterly. Annual subscription: \$30.00. Send subscription orders and remittances for the preceding bibliographic services to National Bureau of Standards, Cryogenic Data Center (275.02) Boulder, Colorado 80302.

U.S. DEPARTMENT OF COMMERCE
National Bureau of Standards
Washington, D.C. 20234

OFFICIAL BUSINESS

Penalty for Private Use, \$300

POSTAGE AND FEES PAID
U.S. DEPARTMENT OF COMMERCE
COM-215



SPECIAL FOURTH-CLASS RATE
BOOK
